


A

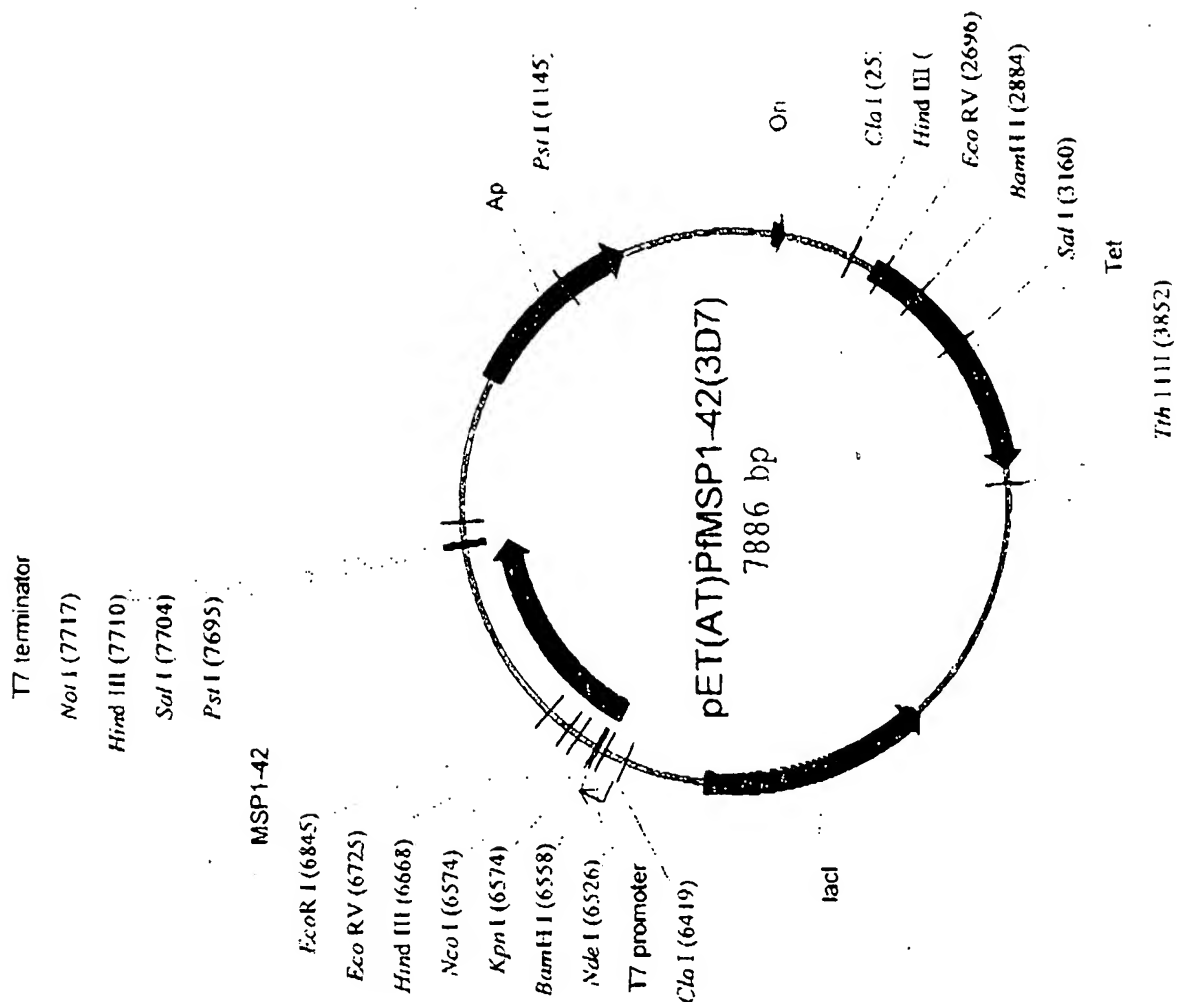

B

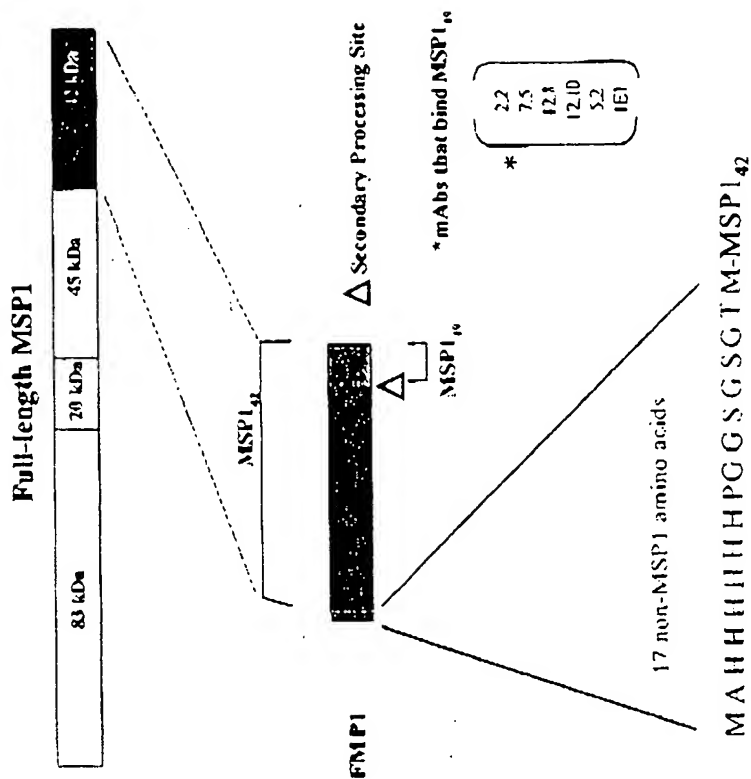


Fig 1

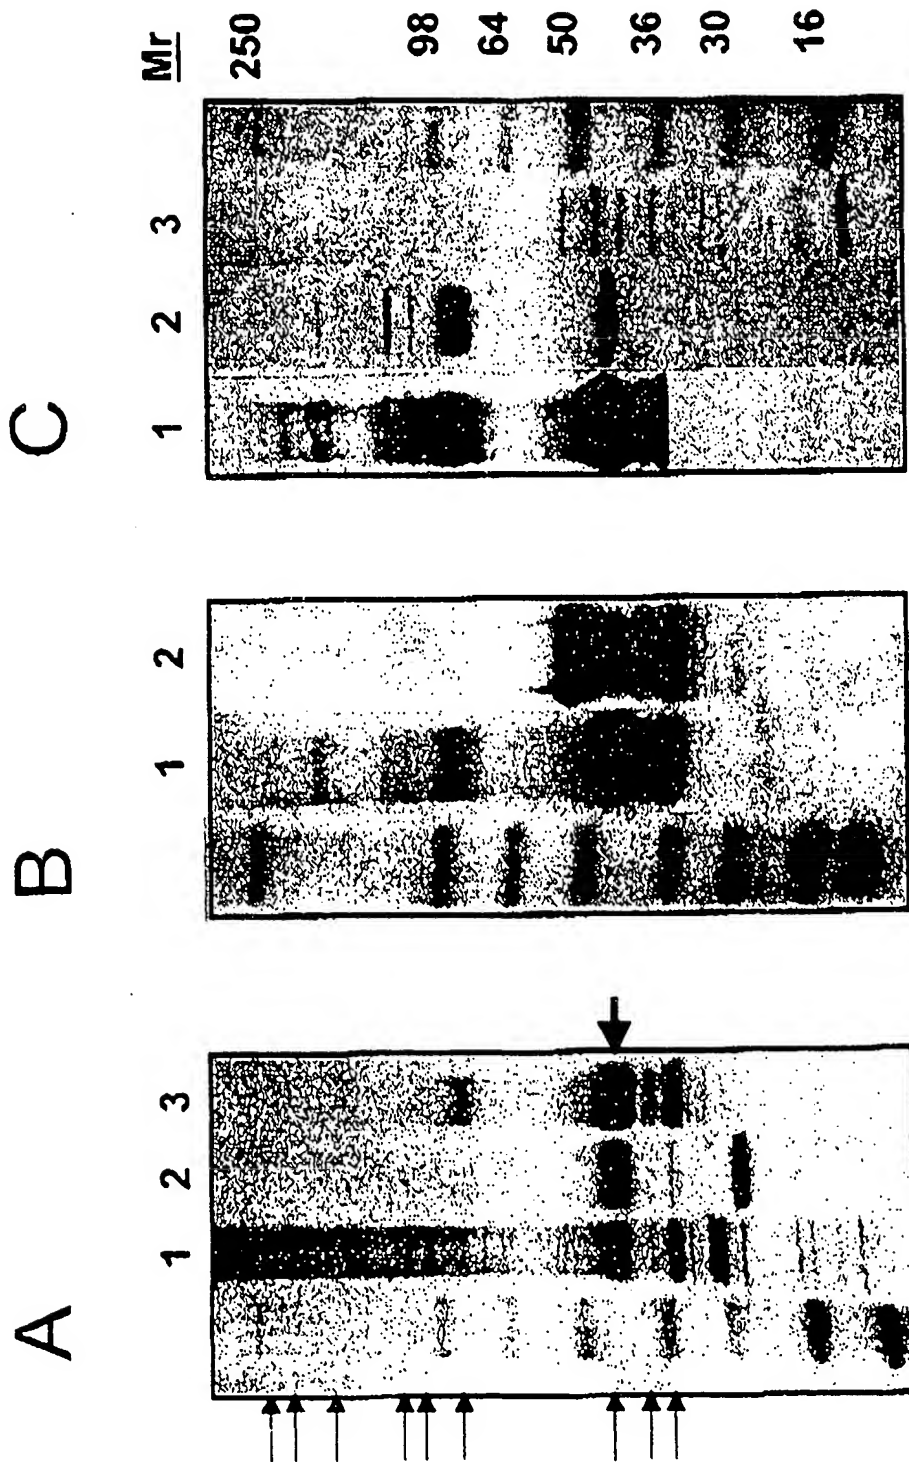
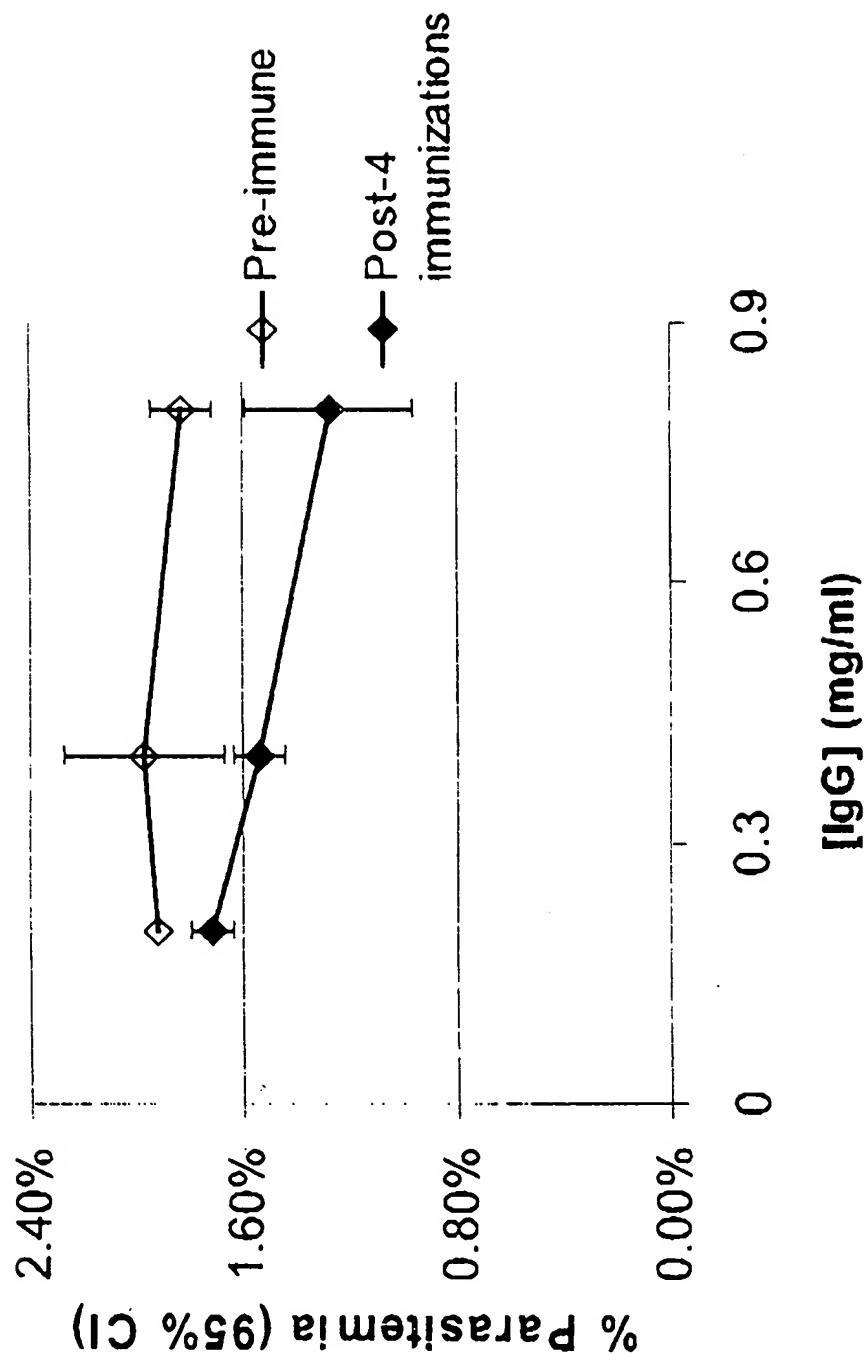


Fig 2



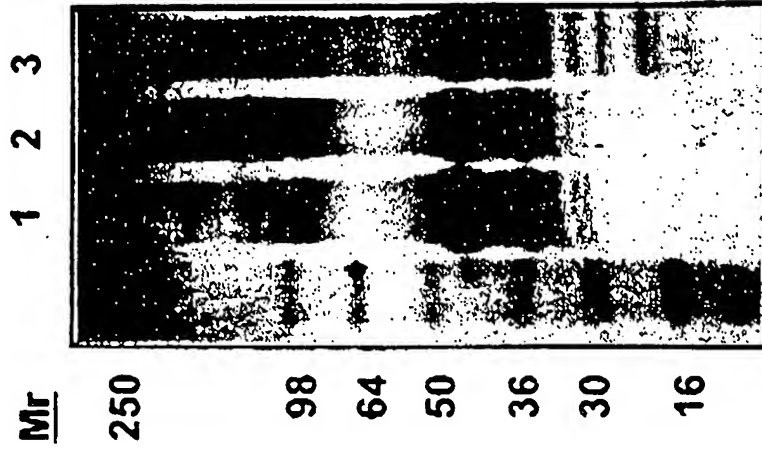


Fig 3


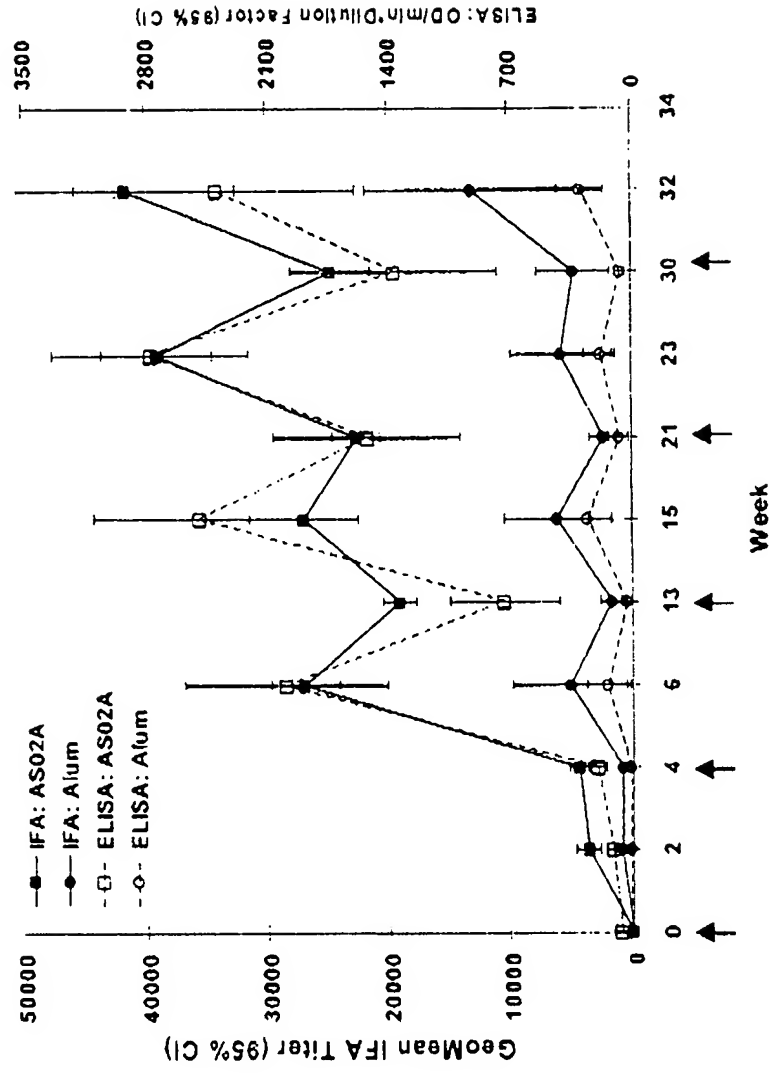


Fig 4

205210" TFS2500T

PBMC stimulated with MSP1₄₂

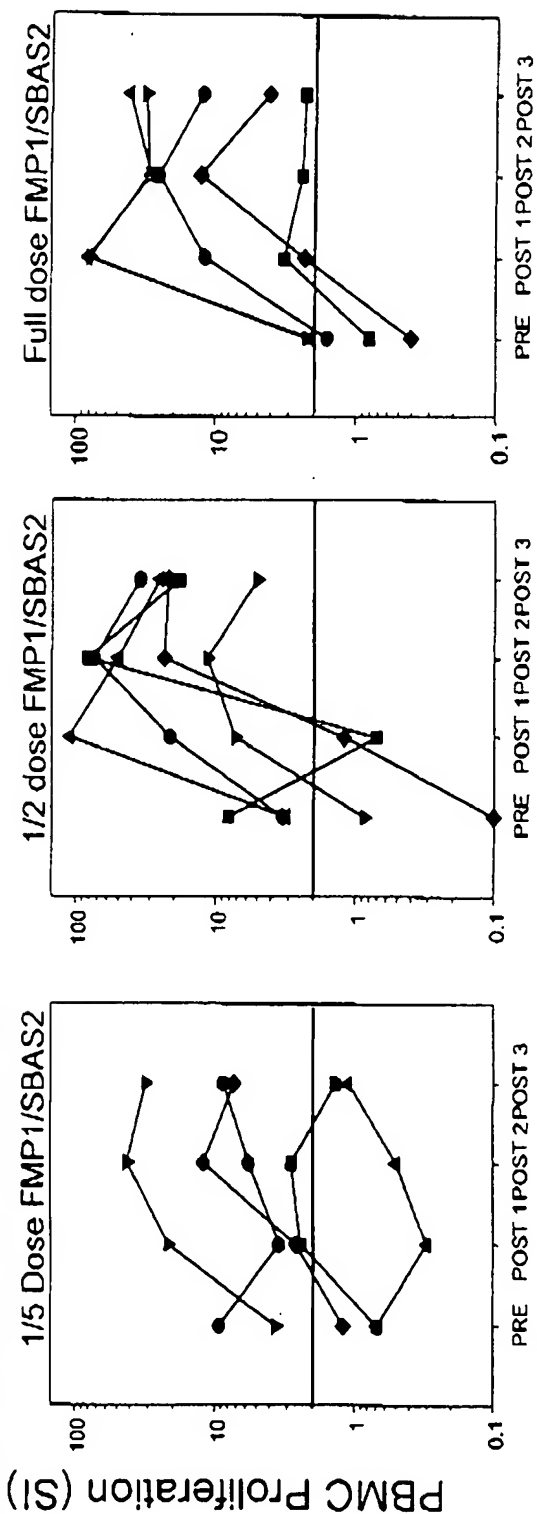

PBMC stimulated with PRBC

